INSTRUCTIONS FOR USE

Long wrist splint

Product code: ManuTim Long

1. Characteristics

Wrist splint is made of breathable material with perforation. Velcro straps provide a snug fit of the stabilizer and firm immobilization.

2. Application

Wrist splint is used to immobilize wrist in functional position ensuring full movement in metacarpophalangeal and interphalangeal joints. The stabilizer relieves wrist bones, joint capsules and tendons.

Indications for use:

- Peritendinitis
- Carpal tunnel syndrome
- Degeneration of wrist joint
- Twists and dislocations
- Overload arthropathy
- After removing plaster cast

Contraindications:

Do not use in case of:

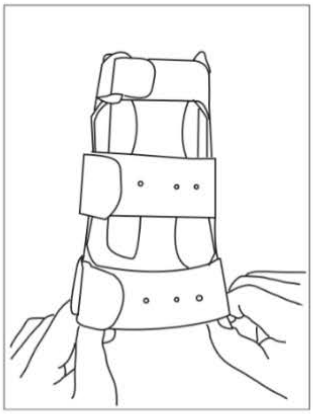
- Skin abrasion
- Eczema
- Wound and other skin injuries
- After application of warming gel or rub
- Individual contraindications which were determined by the doctor during interview and physical examination

3. Notes

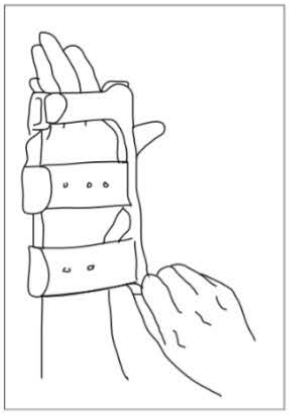
Timago International Group does not bear responsibility of improper maintenance of the product, failure to comply safety regulations and misuse.

4. Fitting instruction

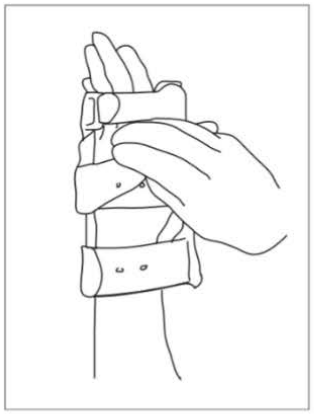
- Before putting, unfasten velcro straps and fasten them again on the loosest clasp (picture 1).
- Place hand into the stabilizer so that the thumb passes through the perforation (picture 2), while velcro straps are on dorsal side (picture 4).
- Adjust and fasten the circumferential strap (picture 3) according to needs.



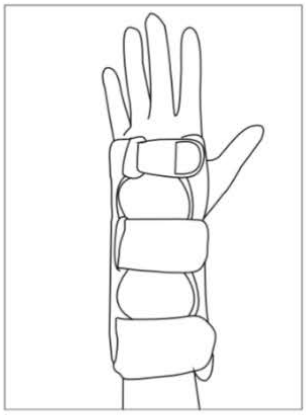
Picture 1



Picture 2



Picture 3



Picture 4

5. Technical data

- The long wrist splint (ManuTim Long) is available in two versions: for left or right hand. Both versions are designed to stabilize the wrist on the side for which they have been anatomically formed. They can’t be used interchangeably.
- Wrist splint length: 26 cm

SIZE	WRIST CIRCUMFERENCE (cm)
XS	10-13
S	13-16
M	16-18
L	18-20
XL	20-23


6. Storage and transport conditions

The product should not be exposed to direct sunlight, water or moisture.

7. Warranty information

All products distributed by our company are covered by a warranty, the terms of which are described in the warranty card available on our website. Please contact the retailer from whom you purchased the product. Please, keep in mind that for warranty purposes, the proof of purchase (receipt or invoice) should be retained.

8. Labels

	Reference number		Manufacturer
	LOT number		Manufacture date
	Serial number		Medical device
	Note		Please read the instruction
	The manufacturer checked for compliance with essential medical devices requirements.		

Our complete line of products is available from our distributors.
Learn more at: **www.timago.com**.
Thank you for choosing Timago!

INSTRUKCJA OBSŁUGI

Długi stabilizator stawu nadgarstkowego
Kod produktu: ManuTim Long

1. Wykonanie

Stabilizator stawu nadgarstkowego wykonany jest z przewiewnego materiału z perforacją. Wykorzystanie systemu rzepów zapewnia ścisłe przyleganie stabilizatora oraz pewne unieruchomienie.

2. Zastosowanie

Stabilizator stawu nadgarstkowego należy do grupy wyrobów medycznych, stosowanych w celu unieruchomienia nadgarstka w pozycji anatomicznej pozwalając na pełny ruch w stawach śródręczno-paliczkowych i między-paliczkowych. Stabilizator zmniejsza obciążenie kości nadgarstka, torebki stawowej oraz ścięgien.

Wskazania do stosowania stabilizatora:

- Zapalenie pochewki ścięgna
- Syndrom kanału nadgarstka
- Zwyrodnienie stawu nadgarstkowego
- Skręcenia i zwichnięcia
- Artropatia przeciążeniowa
- Po zdjęciu opatrunku gipsowego

Przeciwwskazania:

Nie należy stosować w przypadku:

- Otarć naskórka
- Egzem skórnych
- Ran oraz innych uszkodzeń skóry
- Po zastosowaniu żeli i maści rozgrzewających
- Indywidualnych przeciwwskazań, które określone zostały przez lekarza w badaniu podmiotowym i przedmiotowym

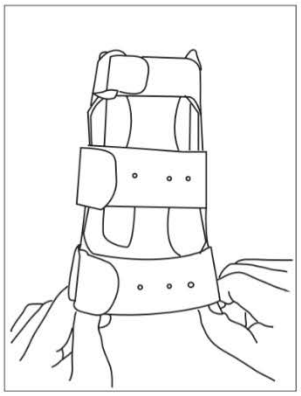
3. Uwagi

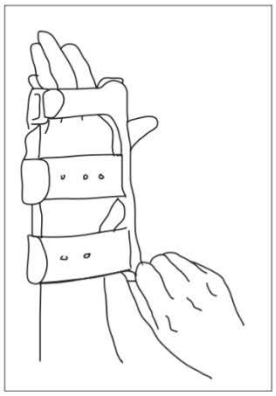
Timago International Group nie ponosi odpowiedzialności za niewłaściwą konserwację wyrobu, nieprzestrzeganie zasad bezpieczeństwa oraz za korzystanie niezgodne z przeznaczeniem.

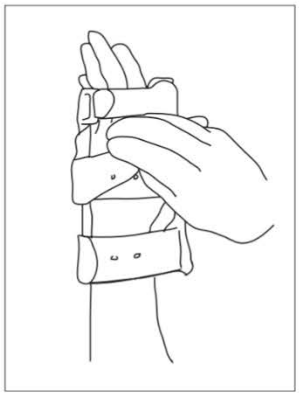
4. Sposób zakładania

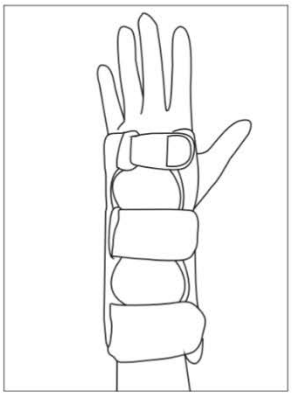
- Przed założeniem należy odpiąć rzepy mocujące i ponowie zapiąć na najluźniejszym mocowaniu (rys. 1).
- Stabilizator należy założyć tak, aby kciuk przechodził przez wycięcie (rys. 2), a rzepy znajdowały się od strony grzbietowej ręki (rys. 4).
- Odpiąć pasy i wyregulować zapięcie (rys. 3) względem potrzeb.

5. Parametry techniczne


Rys. 1


Rys. 2


Rys. 3


Rys. 4

- Długi stabilizator stawu nadgarstkowego (ManuTim Long) występuje w dwóch wersjach: na prawą lub lewą kończynę. Obie wersje przeznaczone są do stabilizacji nadgarstka po stronie, dla której zostały anatomicznie ukształtowane i nie można ich stosować zamiennie.
- Długość stabilizatora: 26 cm

ROZMIAR	OBWÓD NADGARSTKA (cm)
XS	10-13
S	13-16
M	16-18

L	18-20
XL	20-23


6. Warunki przechowywania i transportu

Nie należy narażać wyrobu na bezpośrednie działanie wody i wilgoci.

7. Dane dotyczące gwarancji

Produkt objęty jest gwarancją, której warunki zostały opisane w otrzymanej przez Państwa karcie gwarancyjnej. Do celów gwarancyjnych należy zachować dowód zakupu (paragon lub fakturę).

8. Oznaczenia

	Numer referencyjny		Producent
	Numer serii		Data produkcji
	Numer seryjny		Wyrób medyczny
	Uwaga		Zapoznaj się z instrukcją
	Producent dokonał oceny zgodności z wymogami zasadniczymi dotyczącymi wyrobów medycznych.		

Całość oferty dostępna jest dla Państwa u naszych dystrybutorów. Dowiedz się więcej na **www.timago.com**
Dziękujemy za wybór Timago!



Timago International Group
Spółka z o.o. i Spółka – Spółka komandytowa
ul. Karpacka 24/12
43-316 Bielsko-Biała, Poland

T.: +48 33 499 50 00
F.: +48 33 499 50 11
E.: info@timago.com



01/2024(I)